

CHLORINE DIOXIDE TEST PROCEDURE

The Chlorine Dioxide test procedure utilizes the **STANDARD STRIP METHOD** using the eXact iDip® Smart Photometer System®. For tips on achieving best accuracy, and additional information regarding features of the eXact iDip® photometer and the eXact iDip® app, please refer to the eXact iDip® Smart Guide. You can download a copy on our website at exactidip.com. **Test procedures can vary from test to test. Read full instructions and watch instructional video within the app.**

YOU WILL NEED


- eXact iDip® photometer
- Your smartphone/tablet with the eXact iDip® app installed and Chlorine Dioxide (DPD-1) Cd test purchased in the Store
- (1) eXact® Strip Micro Glycine (Part No. 484014)
- (1) eXact® Strip Micro Chlorine Dioxide (DPD-1) (Part No. 486633)
- Water sample for rinsing and testing



1 SELECT CUSTOMER

- Select **'Customers'** from the Home screen.
- Choose customer from list
OR Tap **'Add customer from contacts'** and choose customer from your contacts list
OR Tap **'+'** to create a new customer
Android users: If no address is found, tap "No addresses found"
- Verify customer has been selected

Note: To take full advantage of the GPS and Data Storage features, each test result must be linked to a contact. Individual users may select their contact listing.

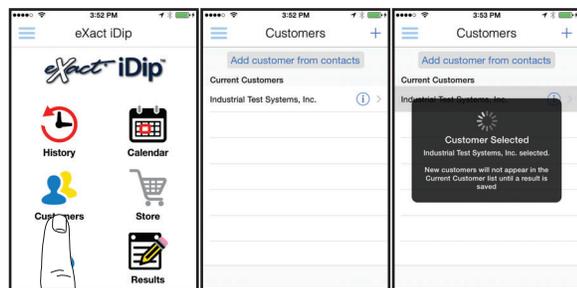

a

b


c

2 POWER ON EXACT IDIP®

Press the **ZERO/ON** button to power on the eXact iDip® photometer.

3 SELECT BLUETOOTH TEST


Tap the menu slide out **'≡'** and select **'Bluetooth Test'** from the choices shown.

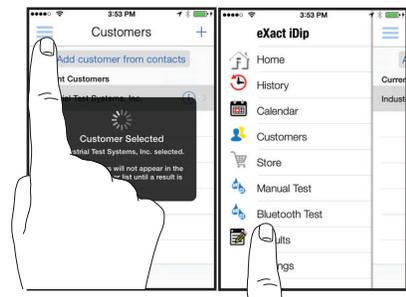

4 CONNECT EXACT IDIP®


The eXact iDip® app will automatically connect to the most recently used eXact iDip® photometer. If not, select your eXact iDip® from the bottom of the screen.

Note: Always connect your eXact iDip® photometer via the Bluetooth® connection within the app. If you experience an issue connecting your device, check that your smartphone/tablet's Bluetooth® is turned on and your device is compatible.

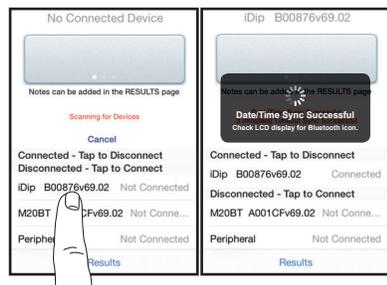

5 SELECT TEST

Tap **'SELECT Test'** at the top and select **Chlorine Dioxide (DPD-1) Cd** (if this is not visible, purchase the test from the Store). The eXact iDip® photometer and eXact iDip® app will both display the test selection for Chlorine Dioxide.

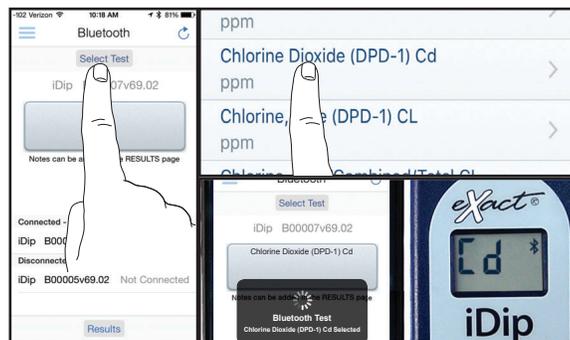

6 FILL CELL

Before testing, rinse CELL and clean with brush thoroughly. Finally, rinse the cell 3 times with the water sample to be tested, then **FILL** cell to capacity to begin test (refer to video in app).



7 REMOVE STRIP

Remove one eXact® Strip Micro Glycine (Part No. 484014) and set in a dry, convenient place. Immediately replace cap on bottle.



8 DIP STRIP

Press **READ** to initiate a 20 second countdown and simultaneously **DIP** the Glycine strip in the sample, gently touching the bottom of the cell. Use a gentle constant back and forth motion (2 strokes per second) until the timer displays "1". Remove and discard the strip.



9 CAP CELL AND ZERO METER

App will show that it is ready to continue with the next part of testing. Tap OK. Press **ZERO/ON** and the eXact iDip® photometer display reads 0PPM indicating the meter is ready for testing.



10 REMOVE STRIP

Remove one eXact® Strip Micro Cd (DPD-1) (Part No. 486633) and set in a dry, convenient place. Immediately replace cap on bottle.



11 DIP STRIP


Press **READ** to initiate another 20 second countdown and simultaneously **DIP** the Cd (DPD-1) test strip in the sample, gently touching the bottom of the cell. Use a gentle constant back and forth motion (2 strokes per second) until the timer displays "1". Remove and discard the strip.

The eXact iDip® photometer will now display a 100 second count-up timer. Make sure your smart device does not go to sleep.



12 CAP CELL AND READ RESULTS

Place the Cell Cover onto the CELL and **READ** result displayed as Chlorine Dioxide. If running multiple tests in a row, repeat steps 5-12.

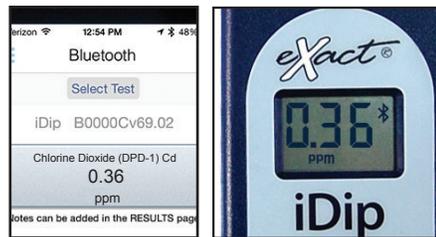

13 CLEAN CELL WITH BRUSH

After testing, rinse CELL immediately and clean with brush to remove reagents which coat the CELL wall.



TIPS

- Due to the manufacturing process, you may find one or two strips that are noticeably smaller or larger in width than the normal strips in the bottle. These should be discarded. Using these strips may give unreliable results.
- Before running test unlock Chlorine Dioxide test by purchasing in the Store.
- To obtain optimal accuracy when testing in direct sunlight, use the Cell Cover when zeroing and reading the sample.
- It is recommended to use the Cell Cleaning Brush with water to clean the CELL after each test to remove reagents which coat the CELL wall.
- Be careful while dipping the strip (steps 8 & 11). Do not spill the sample from the CELL.

MANAGE YOUR RESULTS

Save, send, and share results instantly using the eXact iDip® app. For step-by-step instructions, refer to the eXact iDip® Smart Guide. You can download a pdf copy on-line at exactidip.com.

